


# ICP

## Inductively Coupled Plasma - Optical Emission Spectrometer (ICP-OES)

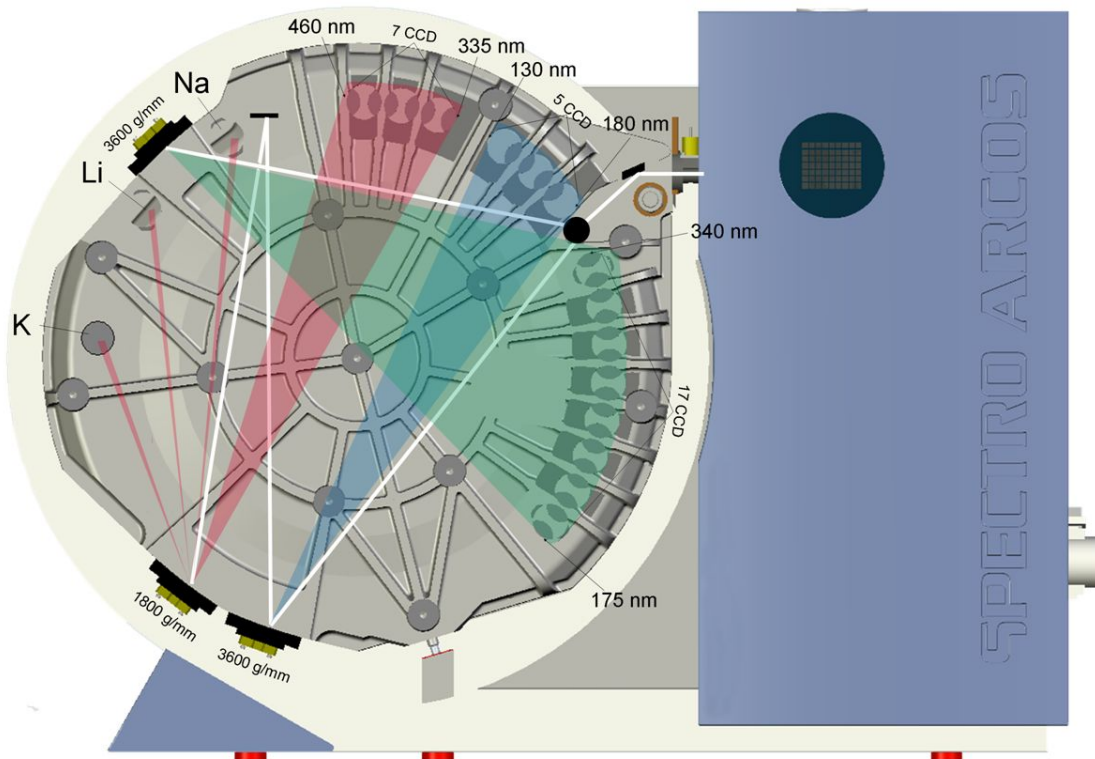

Installation and Operation Tutorials: [ICP Installation](#)

[Vision\\_Tutorial\\_2\\_11\\_630.pdf](#)

[Tutorial\\_Backup.pdf](#)

### ICP OPERATION

[ICP Theory - SPECTRO\\_ARCOS\\_OPTIC\\_Imagefinal.pdf](#)

[Spectro Training ICP](#)

[Changing the Nebulizer](#)

[Using the Transient setting](#)

[ICP Standards](#)

[ICP Commands](#)

[?Exporting Data](#)

[Questions](#)

[Troubleshooting](#)

[Logging onto fileserver1 from ICP computer](#)

[PowerPoint Instructions on using the ICP at Colby](#)

1. Start up
2. ICAL

3. Making Standards
4. Shutdown
5. Cleaning
6. Pump Tubes

Translating NetCDF files generated in transient Mode